

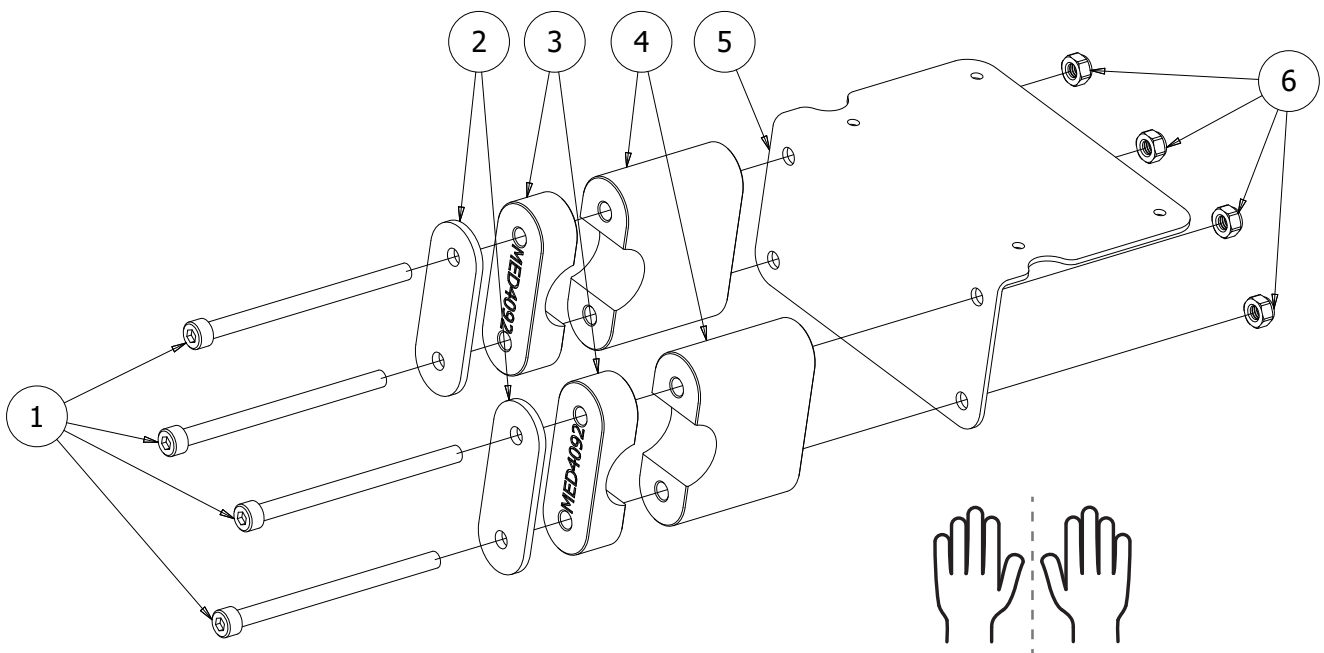
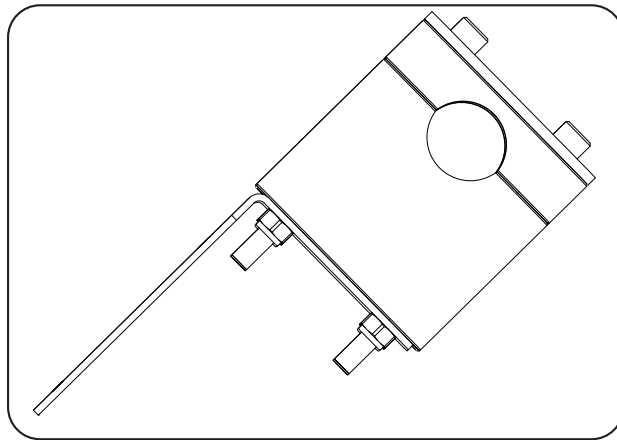



## MED1753


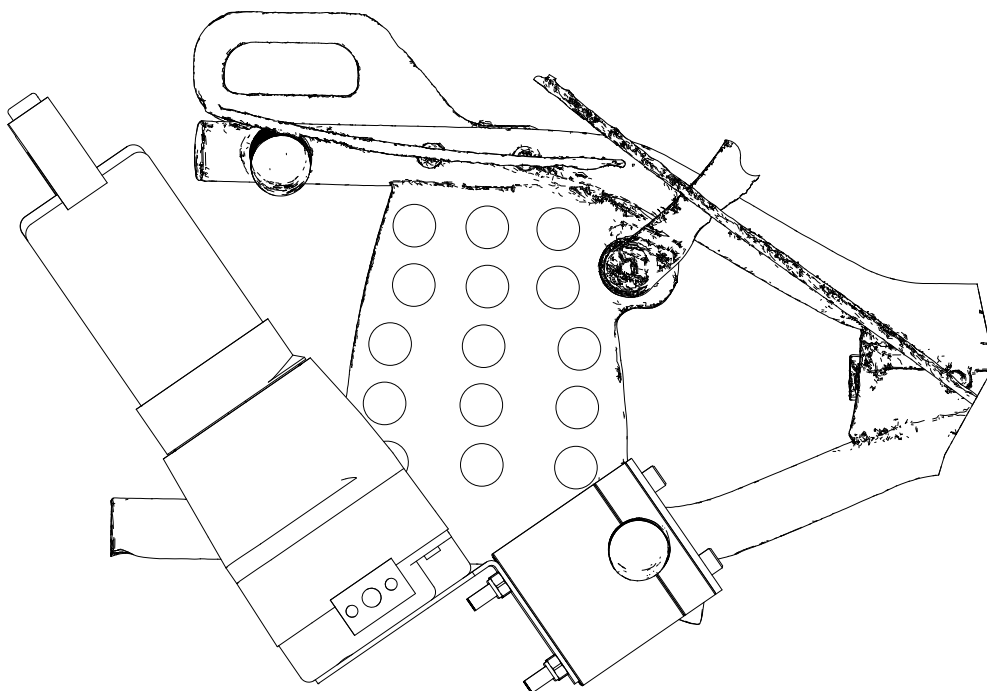



|   |           |   |                                                                                       |
|---|-----------|---|---------------------------------------------------------------------------------------|
| 1 | MC6SM6X90 | 4 |   |
| 2 | MED4093   | 2 |  |
| 3 | MED4092   | 2 |  |
| 4 | MED4091   | 2 |  |
| 5 | MEM5011   | 1 |  |
| 6 | XSM6ML    | 4 |  |

MK Medizintechnik Gmbh - MK Nuage

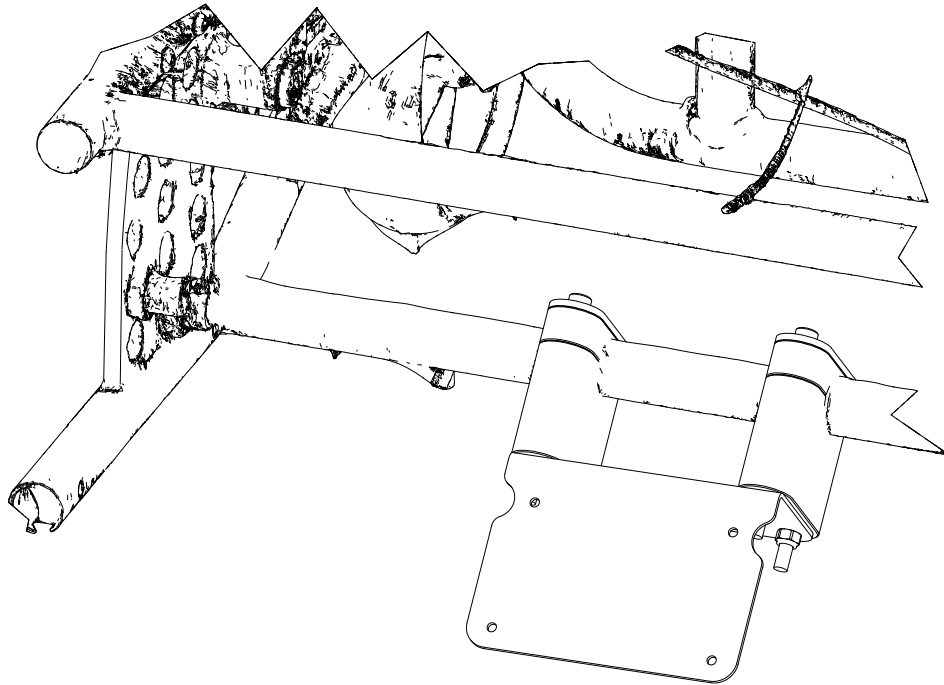

## Netti - AdaptPro

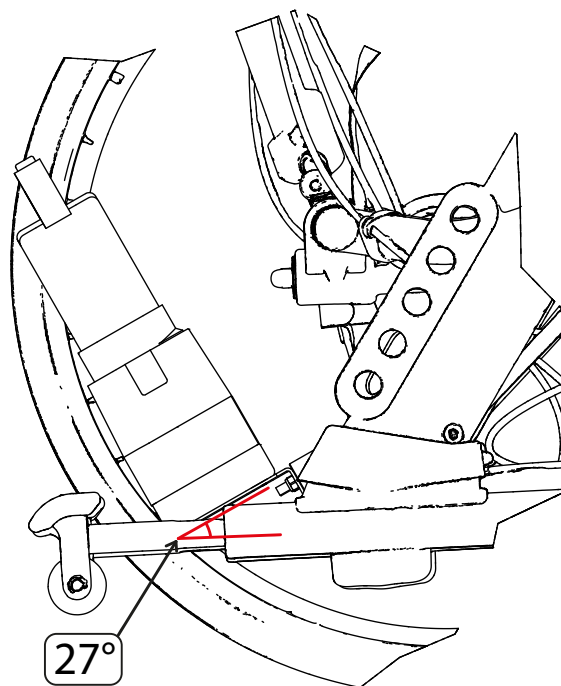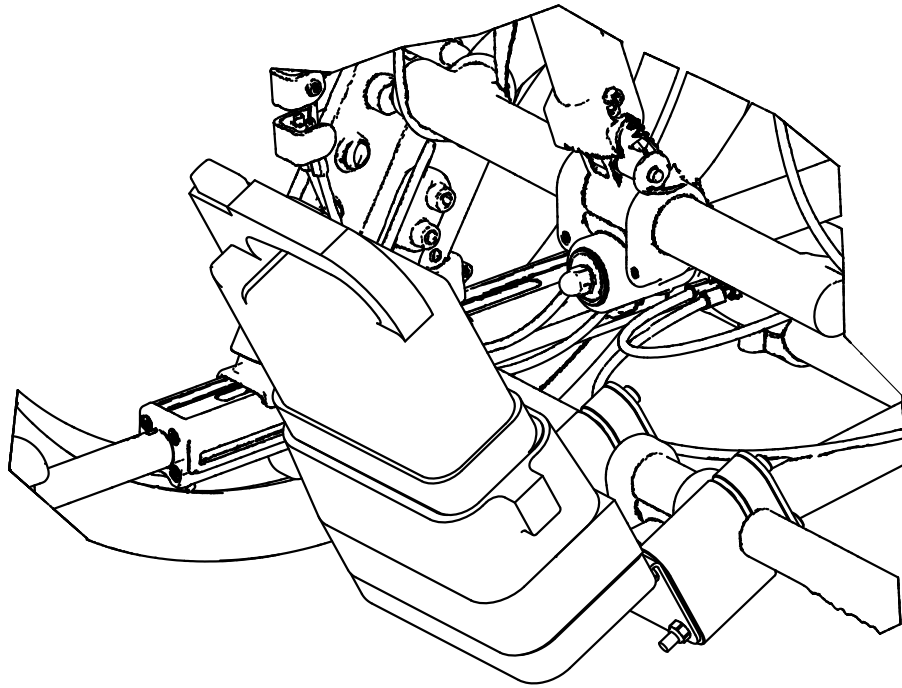

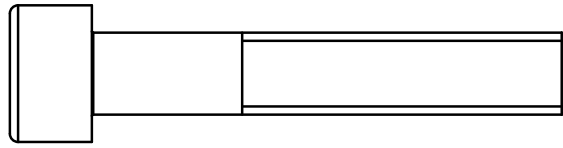

|     |        |
|-----|--------|
| M3  | 1.2 Nm |
| M4  | 3 Nm   |
| M5  | 6 Nm   |
| M6  | 10 Nm  |
| M8  | 25 Nm  |
| M10 | 50 Nm  |
| M12 | 85 Nm  |